

E-DWT Power Supply Replacement Kit

P/N 3622351

Instruction Sheet

Power Supply Replacement kit for E-DWT, P/N 3622351, includes:

DESCRIPTION	QTY	PART NO.
12 V power supply (MFG P/N TR9CE3350LCP-Y)	1	3335610
E-DWT to RPM4, power cable	1	3335955

Introduction

This kit is intended to provide a new power supply and cable for E-DWT. It replaces MFG P/N TR9CE3350CCP-Y with correct power supply MFG P/N TR9CE3350LCP-Y.

Procedure

- ① Vent the unit and disconnect the power cable.
- ② Remove all external cables and plumbing connected to the unit.
- ③ Plug test port, close reservoir vent, and make sure reservoir lid is tightened. (See Figure 1)

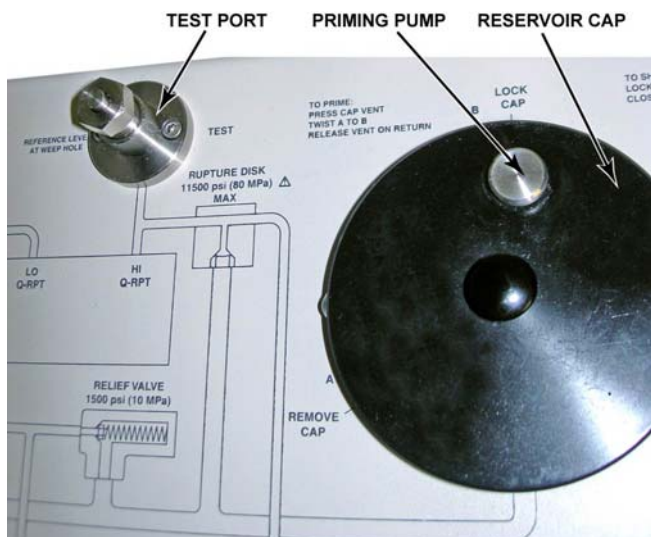


Figure 1: E-DWT top view

- ④ Remove one of the four variable volume handles to allow the E-DWT to be placed on its side.



Figure 2: E-DWT on its side with one handle removed

- ⑤ Locate the 12V power supply connection on the rear housing of the E-DWT. This connection and the internal cable will be replaced. (See Figure 3)



Figure 3: E-DWT rear view detail: power supply connection

- ⑥ Loosen the hex nut using a 3/8 inch socket. If recessed area is too small to allow the socket to fit, use needle nose pliers.

- 7 Locate the internal 12V cable that connects to the RPM4 (see Figure 4).

12V GREY POWER CABLE



Figure 4: E-DWT internal view detail:
12V grey power cable

- 8 Loosen the knurled nut and disconnect the cable from the RPM4. (see Figure 5)

KNURLED NUT



Figure 5: E-DWT internal view detail:
knurled nut to RPM4

- 9 Install the new cable.
- 10 Connect the new cable (knurled nut end) to the RPM4. (see Figure 5) Secure it by manually tightening finger tight.
- 11 Remove the hex nut and washer from the heat-shrunk connector, (see Figure 4) insert the connector through the E-DWT housing, and secure it to the outside of the housing using the washer and hex nut that was just removed. The washer should be installed on the outside of the housing directly under the nut. It is recommended to use Loctite 222MS or similar on the nut to help ensure it does not come loose.
- 12 Reposition the E-DWT on the table in its normal upright position.
- 13 Replace the variable volume handle that was removed. (see Figure 2)
- 14 Connect new power supply and open vent on reservoir for normal operation. (see Figure 1)
- 15 Test functionality to ensure there are no problems with the cable installation or power supply.
- 16 Dispose of old cable and old power supply.

Fluke. Keeping your world up and running.®

Fluke Corporation
DH Instruments Division
4765 East Beautiful Lane
Phoenix, AZ 85044-5318 USA
Ph: 602.431.9100
Fax: 602.431.9559

Fluke Europe B.V.
PO Box 1186, 5602 BD
Eindhoven, The Netherlands

For more information call:
In the U.S.A. (800) 443-5853 or
Fax (425) 446-5116
In Europe/M-East/Africa +31 (0) 40 2675 200 or
Fax +31 (0) 40 2675 222
In Canada (800)-36-FLUKE or
Fax (905) 890-6866

From other countries: +1 (425) 446-5500 or
Fax +1 (425) 446-5116
Web access: <http://www.dhinstruments.com>

©2010 Fluke Corporation. Specifications subject to change without notice. E-DWT-H and E-DWT are registered trademarks of Fluke Corporation, DH Instruments Division.
Printed in U.S.A. 1/2010 3622296A D-EN-N

Modification of this document is not permitted without written permission from Fluke Corporation.