

Q-RPT Replacement Kit

Instruction sheet

This kit includes a replacement Pressure Transducer calibrated to a specific range and class. The kit also contains the following components:

| DESCRIPTION | QTY | PART NO. |
|---|----------------|----------|
| Crimp terminal | 10 | 2207416 |
| Crimp terminal | 10 | 3154579 |
| Crimp terminal | 2 | 3154472 |
| Crimp terminal | 10 | 3154485 |
| Connector | 1 | 2194502 |
| Connector | 1 | 3140008 |
| Connector | 1 | 1812216 |
| Connector | 1 | 3141826 |
| Connector | 1 | 3141173 |
| CRIMP TOOLS (Shown for reference only. Not supplied with kit.) | | |
| PRODUCT | Molex TOOL NO. | |
| PPC4 | 63819-0500 | |
| PPCH and PPCH-G | 63819-0000 | |
| RPM3, molbox, RPM4, PPC3 | 63811-8200 | |

Introduction

Only DHI or DHI Authorized Service Providers are authorized to install replacement Q-RPTs. Replacement or installation by other parties will void the warranty of the Q-RPT and possibly the equipment into which it is installed. Measurement and/or control specifications are also valid only under these conditions.

Q-RPTs are used in a variety of DHI Controllers, Monitors and Flow Terminals. Different crimps, connectors and associated crimp tools are used with different models. The pages that follow show the crimps, connectors and crimp tool required for each equipment type. Refer to the wiring diagrams on the following sheets and to the detailed

instructions included with Molex hand crimp tools, to install crimps onto wires. Molex crimp tool instruction sheets are also available on the Molex website at www.molex.com.

http://www.molex.com/pdm_docs/ats/ATS-638190500.pdf

http://www.molex.com/pdm_docs/ats/ATS-638190000.pdf

http://www.molex.com/pdm_docs/ats/ATS-638118200.pdf

The Molex Quality Crimping Handbook 63800-0029 is also available on Molex website and is a good reference.

http://www.molex.com/pdm_docs/ats/TM-638000029.pdf


Note

DDS NOTE: Some Paroscientific Pressure Transducers include a separate wire bundle used for DIGIQUARTZ DATA STORAGE (DDS). The bundle includes a White/Violet, White/Brown and in some cases a Yellow wire. The DDS wires are utilized only on PPCH, PPCH-G, and PPC4 products. For all other DHI products do not disturb the DDS bundle. Leave it coiled with the wire ends sealed as supplied by Paroscientific.

Wire Lengths: Specific wire lengths have been intentionally omitted from these instructions. Preferred method is to measure the wire length on the existing Transducer being replaced and cut the wire lengths on the replacement Transducer to same length.


Q-RPT must be calibrated after installation.

Connector

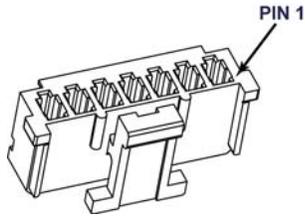


P/N 3141826

Crimp Terminal



P/N 3154579

Crimp Tool

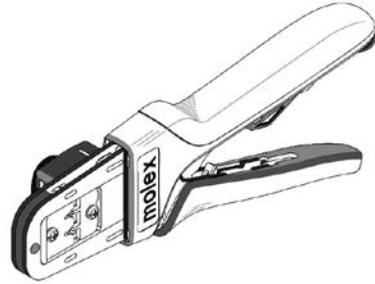

MolPex P/N: 63819-0500


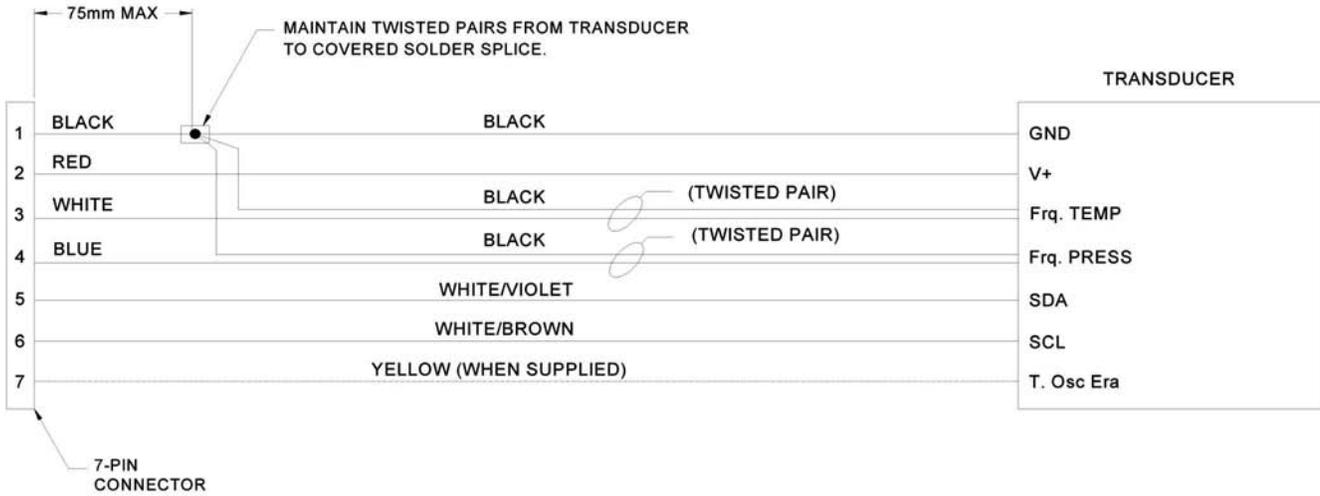



Figure 1: PPC4 Components and Transducer Wiring Diagram

Connector




P/N 2194502

Crimp Terminal

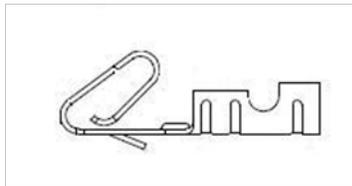

P/N 2207416

Crimp Tool

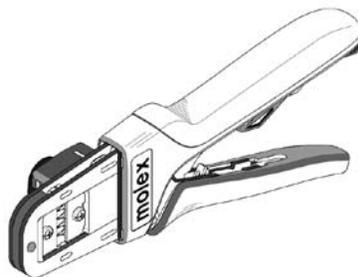

MolPex P/N: 63811-8200


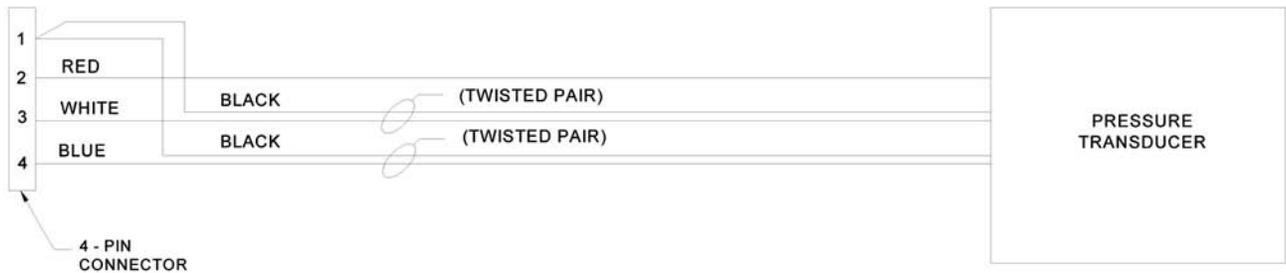



Figure 2: RPM3 Components and Transducer Wiring Diagram

Connector




P/N 1812216

Crimp Terminal

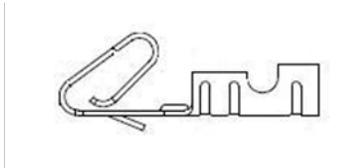

P/N 2207416

Crimp Tool

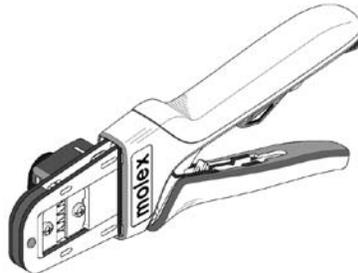

MolPex P/N: 63811-8200


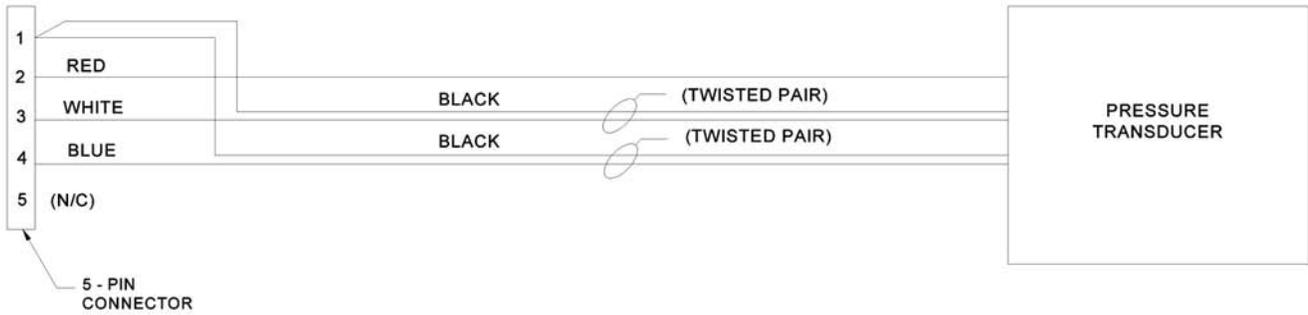



Figure 3: molbox1 and molbox1+ Components and Transducer Wiring Diagram

Connector

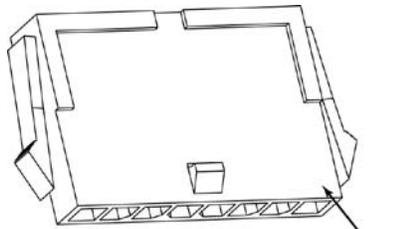


P/N 3141173

Crimp Terminal



P/N 3154472 (1)
 P/N 3154485 (7)
 NOTE: 3154472 HAS LARGER CRIMP BARREL TO ACCEPT MULTIPLE WIRES.

Crimp Tool

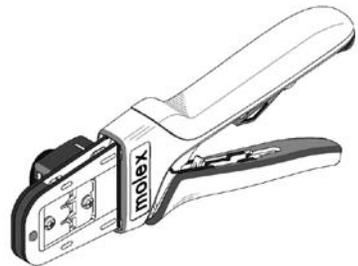

MolPex P/N: 63819-0000


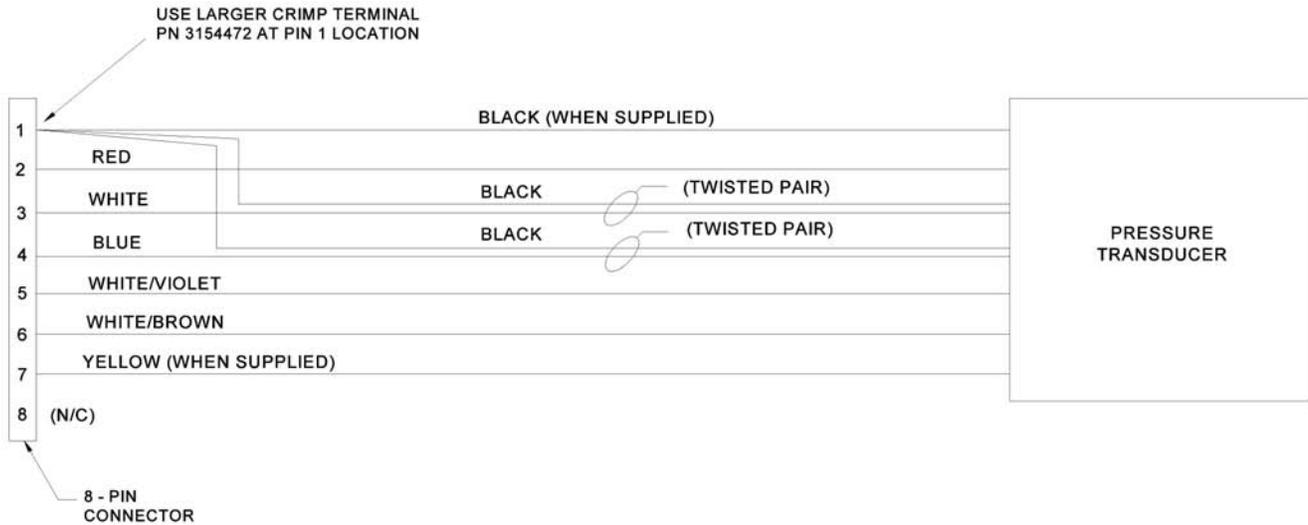



Figure 4: PPCH and PPCH-G Components and Transducer Wiring Diagram

Connector

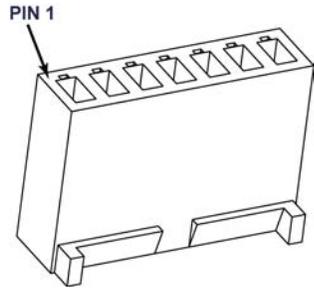


P/N 3140008

Crimp Terminal

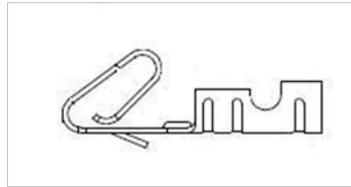

P/N 2207416

Crimp Tool

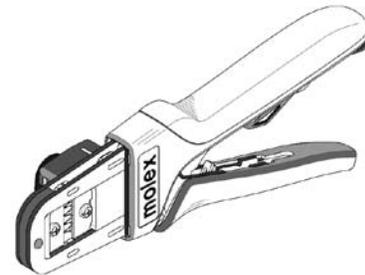

MolPex P/N: 63811-8200

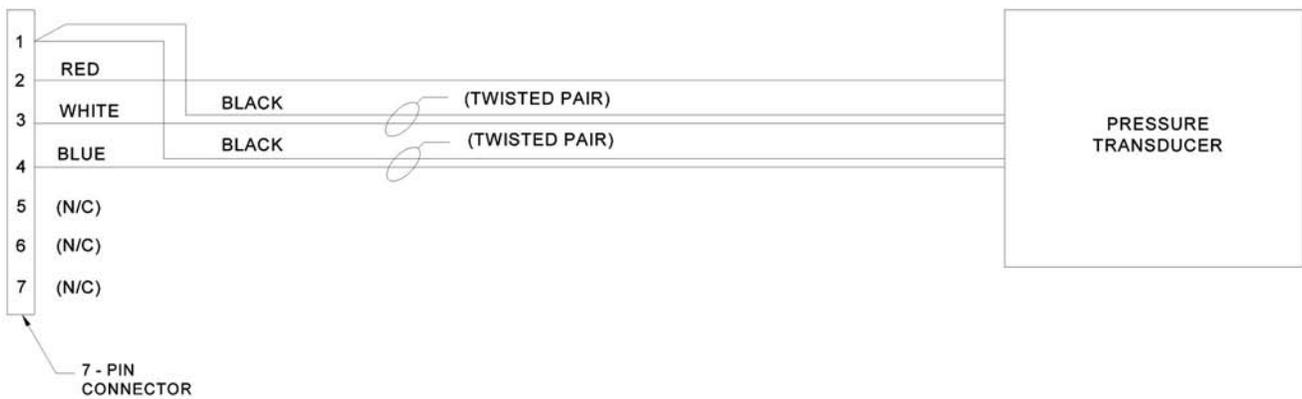


Figure 5: RPM4 and PPC3 Components and Transducer Wiring Diagram

Fluke. Keeping your world up and running.®

Fluke Corporation
DH Instruments Division
 4765 East Beautiful Lane
 Phoenix, AZ 85044-5318 USA
 Ph: 602.431.9100
 Fax: 602.431.9559

Fluke Europe B.V.
 PO Box 1186, 5602 BD
 Eindhoven, The Netherlands

For more information call:
 In the U.S.A. (800) 443-5853 or
 Fax (425) 446-5116
 In Europe/M-East/Africa +31 (0) 40 2675 200 or
 Fax +31 (0) 40 2675 222
 In Canada (800)-36-FLUKE or
 Fax (905) 890-6866

From other countries: +1 (425) 446-5500 or
 Fax +1 (425) 446-5116
 Web access: <http://www.dhinstruments.com>

©2010 Fluke Corporation. Specifications subject to change without notice. E-DWT-H and E-DWT are registered trademarks of Fluke Corporation, DH Instruments Division.
 Printed in U.S.A. 2/2010 3339002A D-EN-N

Modification of this document is not permitted without written permission from Fluke Corporation.